
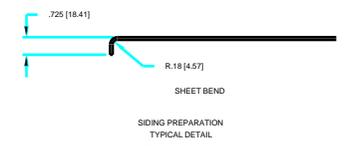
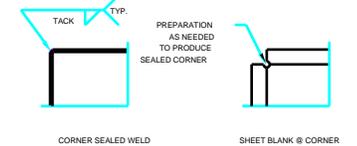
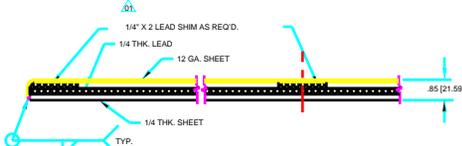
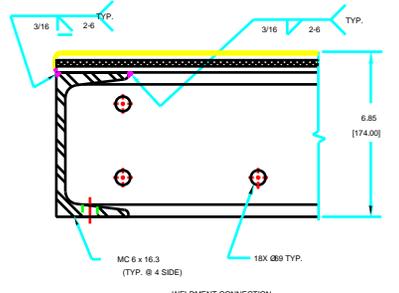


(D) PLOT SCALE: 3/16=1 DWG. SCALE: 1

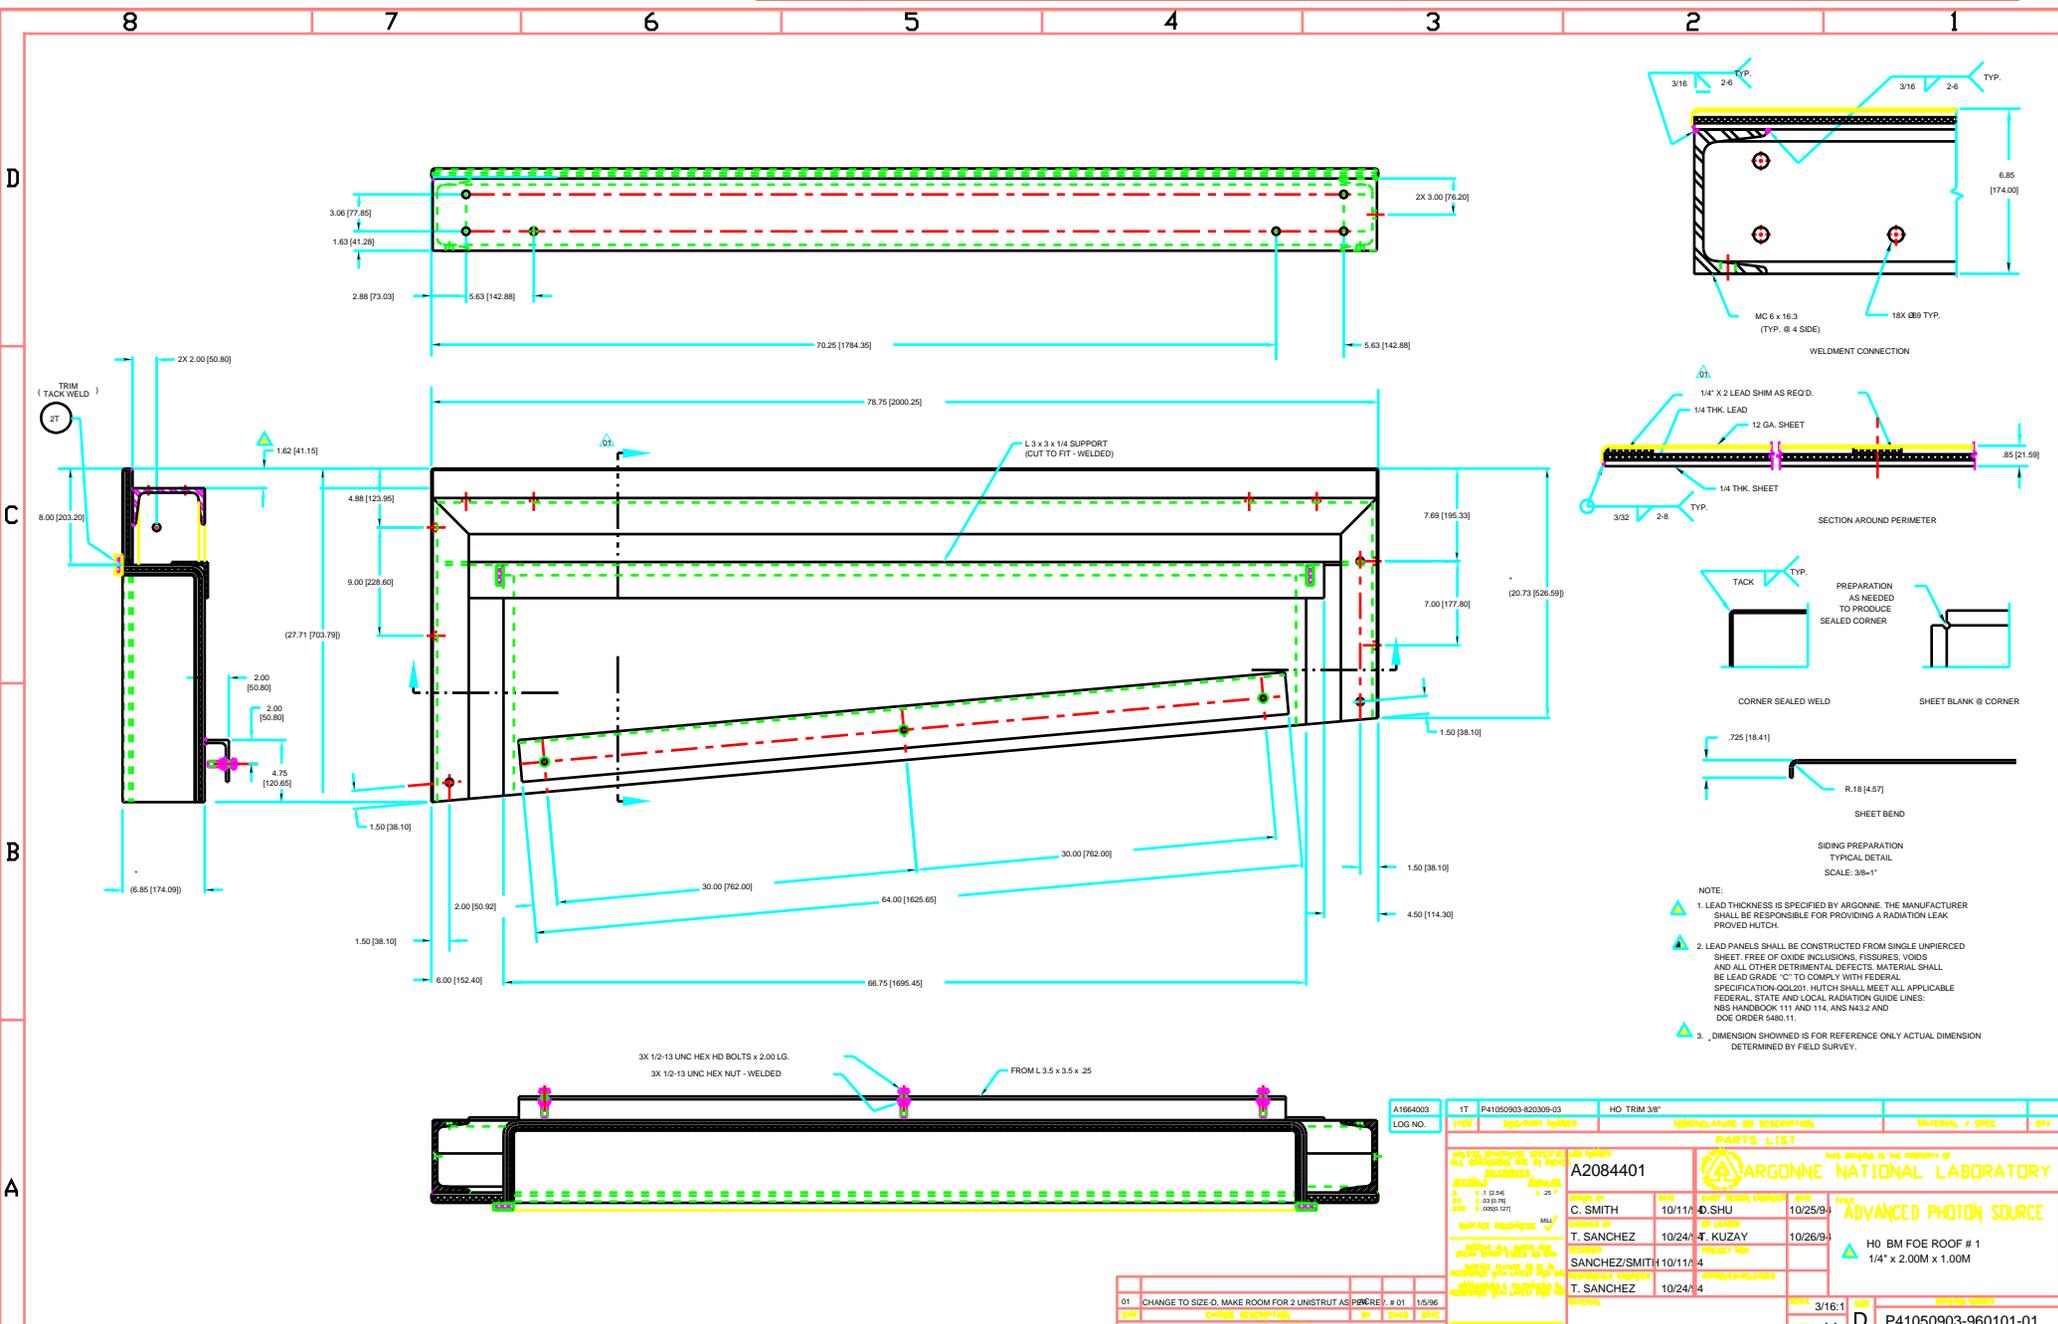

NOTE:
 1. LEAD THICKNESS IS SPECIFIED BY ARGONNE. THE MANUFACTURER SHALL BE RESPONSIBLE FOR PROVIDING A RADIATION LEAK PROOFED HUTCH.
 2. LEAD PANELS SHALL BE CONSTRUCTED FROM SINGLE UNPIERCED SHEET, FREE OF OXIDE INCLUSIONS, FISSURES, VOIDS AND ALL OTHER DETRIMENTAL DEFECTS. MATERIAL SHALL BE LEAD GRADE 'C' TO COMPLY WITH FEDERAL SPECIFICATION QQ-C001. HUTCH SHALL MEET ALL APPLICABLE FEDERAL, STATE AND LOCAL RADIATION GUIDE LINES: NBS HANDBOOK 111 AND 114, ANSI N43.2 AND DOE ORDER 5480.11.
 3. DIMENSION SHOWN IS FOR REFERENCE ONLY ACTUAL DIMENSION DETERMINED BY FIELD SURVEY.

A1664003	1T	P41050903-620309-03	HO TRIM 3/8"		
LOG NO.	ITEM	DESCRIPTION	QUANTITY	UNIT	DATE
PARTS LIST					
A2084401 ADVANCED PHOTON SOURCE HO BM FOE ROOF # 1 1/4" x 2.00M x 1.00M			ARGONNE NATIONAL LABORATORY 10/11/04 T. SANCHEZ		
01	CHANGE TO SIZE-D, MAKE ROOM FOR 2 UNISTRUTS	PW/RE	# 01	1/5/96	
02	CHANGE DESCRIPTION	BY	CHS	DATE	