

SPECIFICATIONS

SHIELDING REQUIREMENTS:

ENTRY PANEL 1"THK LEAD
 BACK WALL 3/8"THK LEAD
 SIDE WALLS 3/8"THK LEAD
 ROOF 1/4"THK LEAD

CONSTRUCTION: MODULAR

STRUCTURE: SELF-SUPPORTED

COMMERCIAL RATED: 40 LBS LIVE WEIGHT/SQ FT
 100 LBS DEAD WEIGHT/SQ FT

OVERALL DIMS:

1.75M Avg WIDTH X 8.75M LONG X 3.3M HIGH [5.8' X 28.7' X 11']
 CLEAR HEIGHT INSIDE: 3M [10']
 DOOR OPENING: 2.4M HIGH X 1M WIDE [8'X 3.3']

SLIDING DOORS: ONE MANUAL, FIXED BY LATCH
 TWO PNEUMATIC WITH MANUAL OVERRIDE

STANDARD SIDE PANEL: 1M WIDE X 3.3M HIGH [3.3'X11']
SANDWICH CONSTRUCTION:
 STEEL 3mm [1/8" (11Ga)] - LEAD 10mm [3/8"]- STEEL 6mm[1/4"]
STRUCTURE: 3" X 3" X 1/4" STEEL ANGLE, ALL AROUND
WEIGHT: 1500LB

STANDARD BACK PANEL: 1M WIDE X 3.3M HIGH [3.3'X11']
SANDWICH CONSTRUCTION:
 STEEL 3mm [1/8" (11Ga)] - LEAD 10mm [3/8"]- STEEL 6mm[1/4"]
STRUCTURE: 3" X 3" X 1/4" STEEL ANGLE, ALL AROUND
WEIGHT: 1500LB

STANDARD ROOF PANEL: 1M WIDE X 1.75M LONG [3.3'X5.8']
SANDWICH CONSTRUCTION:
 STEEL 3mm [1/8" (11Ga)] - LEAD 6mm [1/4"]- STEEL 6mm[1/4"]
STRUCTURE: MC 6 X 3" X 16.3 STEEL CHANNEL, ALL AROUND
WEIGHT: 863LB

STANDARD DOOR PANEL: 1M WIDE X 2.5M HIGH [3.3'X8']
SANDWICH CONSTRUCTION:
 STEEL 3mm [1/8" (11Ga)] - LEAD 10mm [3/8"]- STEEL 6mm[1/4"]
STRUCTURE: 2" X 2" X 1/8" STEEL ANGLE, ALL AROUND
WEIGHT: 886LB


LABYRINTH PANELS: UTILITIES, CABLES, VENTILATION, OZONE

UTILITIES: CHILLED WATER 5°-0.8°C [41°-1.5°F]
 DI WATER
 COMPRESSED AIR 90psi
 ELECTRICAL POWER 30kVA 120/208V

WORK STATION CRANE WITH MANUAL HOIST:

SPAN 1.14M [3.75'] X RUNWAY LENGTH 6.75M [22.15'] X CLEAR HEIGHT 3M [10']
 CAPACITY: 1000Kg [1 TON]

ILLUMINATION: FLUORESCENT- OFFICE RATED: 100 FOOT CANDLE.

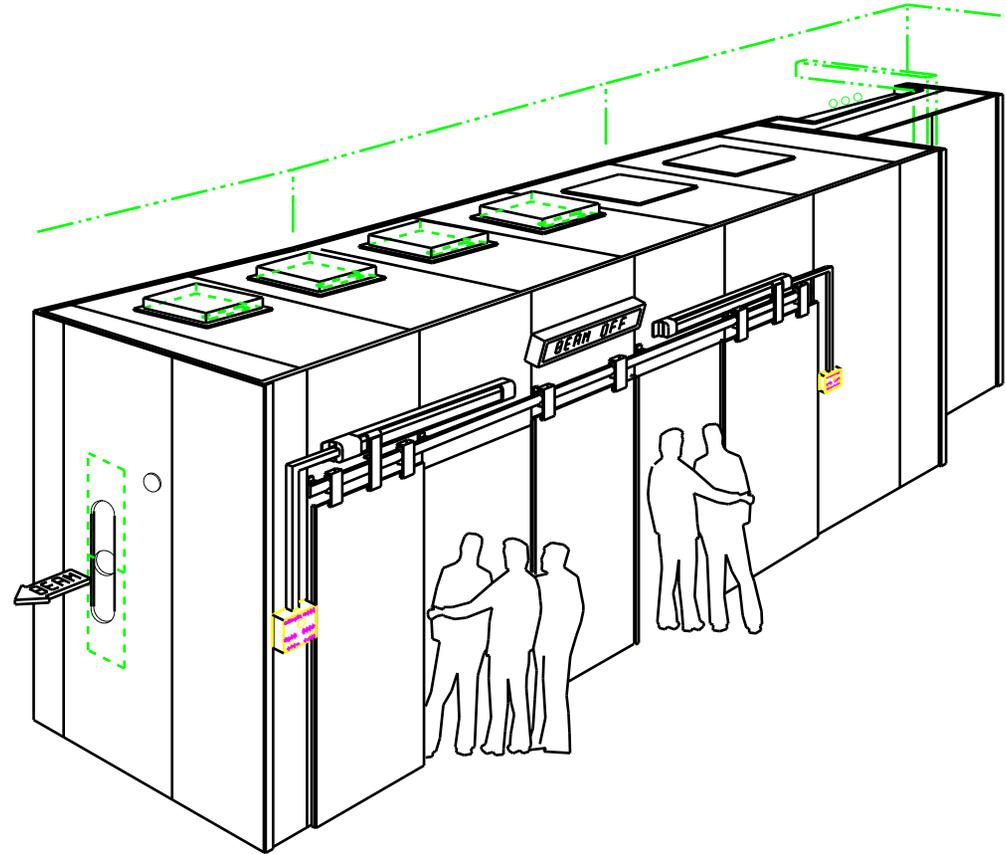

NOTES:

1- THE HUTCH MANUFACTURER SHALL BE RESPONSIBLE FOR THE STRUCTURAL INTEGRITY OF THE HUTCH, AND SHALL CERTIFY THAT THE STRUCTURE WAS REVIEWED BY A LICENSED STRUCTURAL ENGINEER.

STRUCTURES AND THEIR ELEMENTS SHALL BE BUILT FOLLOWING DOE 6430 AS REFERRED TO IN TECHNICAL SPECS. DESIGN LOADS SHALL INCLUDE LOADS THAT CAN OCCUR DURING CONSTRUCTION. DEAD LOADS SHALL INCLUDE THE USE OF THE INTERIOR UNISTRUT FOR SHELVES ONE FOOT WIDE SUPPORTING LOADS OF 200 LBS.

2- LEAD THICKNESS IS SPECIFIED BY ARGONNE. THE MANUFACTURER SHALL BE RESPONSIBLE FOR PROVIDING A RADIATION LEAK PROOF HUTCH.

LEAD LINED PANELS SHALL BE CONSTRUCTED FROM SINGLE UNPIERCED SHEET, FREE OF OXIDE INCLUSIONS, FISSURES, VOIDS AND ALL OTHER DETRIMENTAL DEFECTS. MATERIAL SHALL BE LEAD GRADE 'C' TO COMPLY WITH FEDERAL SPECIFICATION QQ-L-201. HUTCH SHALL MEET ALL APPLICABLE RADIATION GUIDE LINES REFERRED TO IN TECHNICAL SPECS.

REV	DESCRIPTION	DATE	BY	CHKD	APP'D
01	UPDATED & ADDED SHTS. 3-10		RJK		
02	REVISED TECHNICAL SPECIFICATIONS		RJK		

NO.	QUANTITY	DESCRIPTION	UNIT	REVISION
1	1	ENCLOSURE		
2	1	DOOR		
3	1	CRANE		
4	1	HOIST		
5	1	ROOF PANEL		
6	1	BACK PANEL		
7	1	SIDE PANEL		
8	1	ENTRY PANEL		
9	1	LABYRINTH PANEL		
10	1	WORK STATION		
11	1	ILLUMINATION		

NO.	NAME	DATE	REVISION
1	A. TORRES	4/20/09	1
2	D. SHU	4/21/04	1
3	T.M. KLIZAY	4/21/04	1
4	D. MULLS	4/21/04	1
5	T. SANCHEZ	4/20/09	1

PROJECT NO.	A1843001
PROJECT NAME	ARGONNE NATIONAL LABORATORY
PROJECT LOCATION	ADVANCED PHOTON SOURCE
PROJECT DESCRIPTION	H1 FOE 1-BM-A
PROJECT STATUS	FIRST OPTICS ENCLOSURE ASSY.
PROJECT SPECIFICATIONS	(PERSPECTIVE & SPECIFICATIONS)
PROJECT NUMBER	P41050903-330000-01