

SPECIFICATIONS

SHIELDING REQUIREMENTS:

- BACK WALL 2" THK LEAD
- SIDE WALL 3/4" THK LEAD
- ROOF 1/2" THK LEAD

CONSTRUCTION: MODULAR

STRUCTURE: SELF-SUPPORTED

- COMMERCIAL RATED: 40LBS LIVE WEIGHT/SQ FT
- 100 LBS DEAD WEIGHT/SQ FT

OVERALL DIMS: 1.75M Ave WIDE X 8.54M LONG X 3.3M HIGH [5.8' X 28' X 11']

- CLEAR HEIGHT INSIDE: 3M [10']
- DOOR OPENING: 2.4M HIGH X 1M WIDE [8' X 3.3']

SLIDING DOORS:

- ONE MANUAL, FIXED BY LATCH
- ONE PNEUMATIC WITH MANUAL OVERRIDE

STANDARD SIDE PANEL: 1M WIDE X 3.3M HIGH [3.3'X11']

- CONSTRUCTION: SANDWICH : STEEL 3mm [1/8" (11Ga)] - LEAD 19mm [3/4"] - STEEL 6mm[1/4"]
- STRUCTURE: 3 1/2" X 3 1/2" X 1/4" STEEL ANGLE, ALL AROUND
- WEIGHT: 2280LB

STANDARD BACK PANEL: 1M WIDE X 3.3M HIGH [3.3'X11']

- CONSTRUCTION: SANDWICH : STEEL 3mm [1/8" (11Ga)] - LEAD 50mm [2"] - STEEL 6mm[1/4"]
- STRUCTURE: 3 1/2" X 3 1/2" X 1/4" STEEL ANGLE, ALL AROUND
- WEIGHT: 5680LB

STANDARD ROOF PANEL: 1M WIDE X 1.75M LONG [3.3'X5.8']

- CONSTRUCTION: SANDWICH : STEEL 3mm [1/8" (11Ga)] - LEAD 13mm [1/2"] - STEEL 6mm[1/4"]
- STRUCTURE: MC 6 X 16.3 STEEL CHANNEL, ALL AROUND
- WEIGHT: 1150LB

STANDARD DOOR PANEL: 1M WIDE X 2.5M HIGH [3.3'X8']

- CONSTRUCTION: SANDWICH : STEEL 3mm [1/8" (11Ga)] - LEAD 19mm [3/4"] - STEEL 6mm[1/4"]
- WEIGHT: 1470LB

LABYRINTH PENETRATIONS: UTILITIES, CABLES, VENTILATION, OZONE


UTILITY LABYRINTH: CHILLED WATER 5°-0.8°C [41°-1.5°F]

- DI WATER
- COMPRESSED AIR 103 5psi
- ELECTRICAL POWER 30kVA 120/208V

WORK STATION CRANE WITH MANUAL HOIST

- SPAN 1.21M [4.00'] X RUNWAY LENGTH 8.15M [26.75'] X CLEAR HEIGHT 3.00M [10']
- CAPACITY: 1000Kg [1 TON]

ILLUMINATION: FLUORESCENT - OFFICE RATED: 100 FOOT CANDLE.

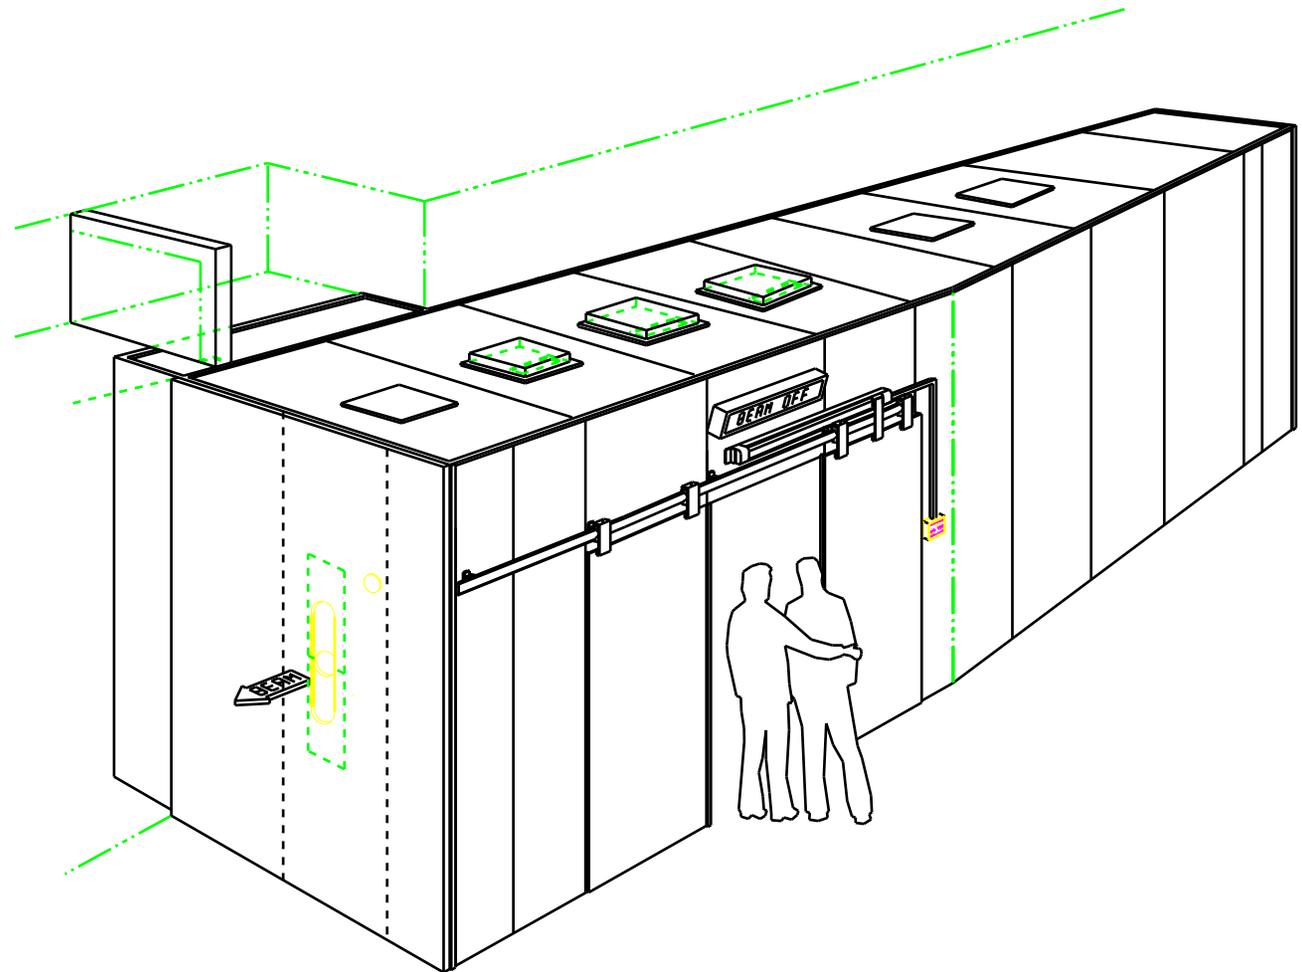

NOTES:

1- THE HUTCH MANUFACTURER SHALL BE RESPONSIBLE FOR THE STRUCTURAL INTEGRITY OF THE HUTCH, AND SHALL CERTIFY THAT THE STRUCTURE WAS REVIEWED BY A LICENSED STRUCTURAL ENGINEER.

STRUCTURES AND THEIR ELEMENTS SHALL BE BUILT FOLLOWING DOE 6430 AS REFERRED TO IN TECHNICAL SPECS. DESIGN LOADS SHALL INCLUDE LOADS THAT CAN OCCUR DURING CONSTRUCTION. DEAD LOADS SHALL INCLUDE THE USE OF THE INTERIOR UNISTRUT FOR SHELVES ONE FOOT WIDE SUPPORTING LOADS OF 200 LBS.

2- LEAD THICKNESS IS SPECIFIED BY ARGONNE. THE MANUFACTURER SHALL BE RESPONSIBLE FOR PROVIDING A RADIATION LEAK PROOF HUTCH.

LEAD LINED PANELS SHALL BE CONSTRUCTED FROM SINGLE UNPIERCED SHEET, FREE OF OXIDE INCLUSIONS, FISSURES, VOIDS AND ALL OTHER DETRIMENTAL DEFECTS. MATERIAL SHALL BE LEAD GRADE 'C' TO COMPLY WITH FEDERAL SPECIFICATION QQ-L-201. HUTCH SHALL MEET ALL APPLICABLE RADIATION GUIDE LINES REFERRED TO IN TECHNICAL SPECS.

02	TO COMPLETE ASSY DRAWINGS	ACRR			
01	UPDATED	ES	TS	CS	CS

REV	DESCRIPTION	DATE	BY	CHKD	APP'D
01	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
02	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
03	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
04	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
05	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
06	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
07	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
08	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
09	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09
10	ISSUED FOR CONSTRUCTION	4/20/09	T. TORRES	D. SHU	4/21/09

ARGONNE NATIONAL LABORATORY
 ADVANCED PHOTON SOURCE
 H1 APS WBE 3-ID-B
 WHITE BEAM EXPERIMENTAL
 STATION ASSEMBLY
 (PERSPECTIVE & SPEC.)

P41050903-620000-02